





Active Circumferential Graft Compression
from the joint space to the cortex

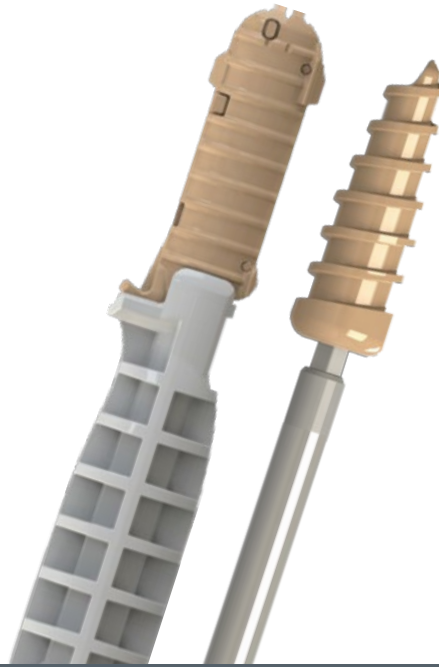



Anatomic Reconstruction
of the Native Tibial Footprint

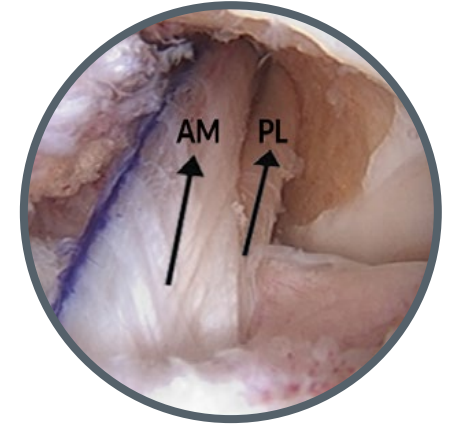

AperFix® II Tibial Sheath & Screw System

The all PEEK-OPTIMA® AperFix® II Cannulated Tibial System allows for precise anatomic positioning of the tibial graft and delivers **class-leading strong, rigid fixation**¹.

Less than 1% Revision Rate at 2 Years,
confirmed by multiple, peer reviewed articles.^{1,2}

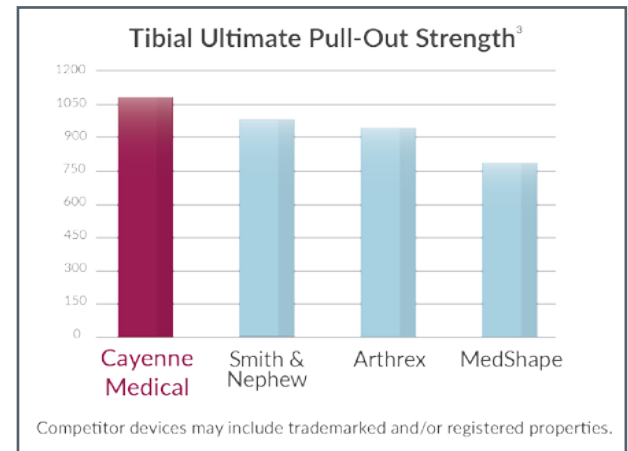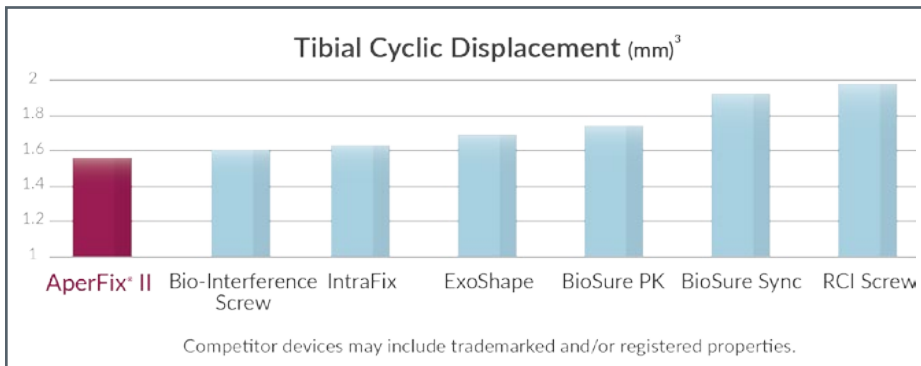

These products are covered by one or more U.S. patents.



Cayenne Medical, Inc.
16597 North 92nd St, Suite 101 | Scottsdale, AZ 85260
cayennemedical.com | 1-888-229-3661

All-inclusive tibial system provides everything needed in one box for a **fast and simple procedure**.



AperFix® II Tibial Sheath & Screw System

AperFix® II Tibial Sheath & Screw System (Sterile)	
Model #	Item Description
CM-3008	AperFix® II Tibial System with Driver, 8mm x 30mm
CM-3009C	AperFix® II Cannulated Tibial System with Driver, 9mm x 30mm
CM-3010C	AperFix® II Cannulated Tibial System with Driver, 10mm x 30mm
CM-3011C	AperFix® II Cannulated Tibial System with Driver, 11mm x 30mm

References:

1. Uribe JW, Arango D, Frank J, Kiebzak GM. Two-year Outcome With the AperFix System for ACL Reconstruction. *Orthopedics*. 2013; 36(2): 159-164.
2. G Görmeli, CA Görmeli, M Karakaplan, MF Korkmaz, U Diliçikık, H Gözükar. Outcome of transtibial AperFix system in anterior cruciate ligament injuries. *Indian J Orthop*. 2015 Mar-Apr; 49(2): 150-154.
3. Aga C, Rasmussen MT, Smith SD, Jansson KS, LaPrade RF, Engebretsen L, Wijdicks CA. Biomechanical Comparison of Interference Screws and Combination Screw and Sheath Devices for Soft Tissue Anterior Cruciate Ligament Reconstruction on the Tibial Side. *Am J Sports Med*. 2013 Apr;41(4):841-8.

These products are covered by one or more U.S. patents.



Cayenne Medical, Inc.
16597 North 92nd St, Suite 101 | Scottsdale, AZ 85260
cayennemedical.com | 1-888-229-3661